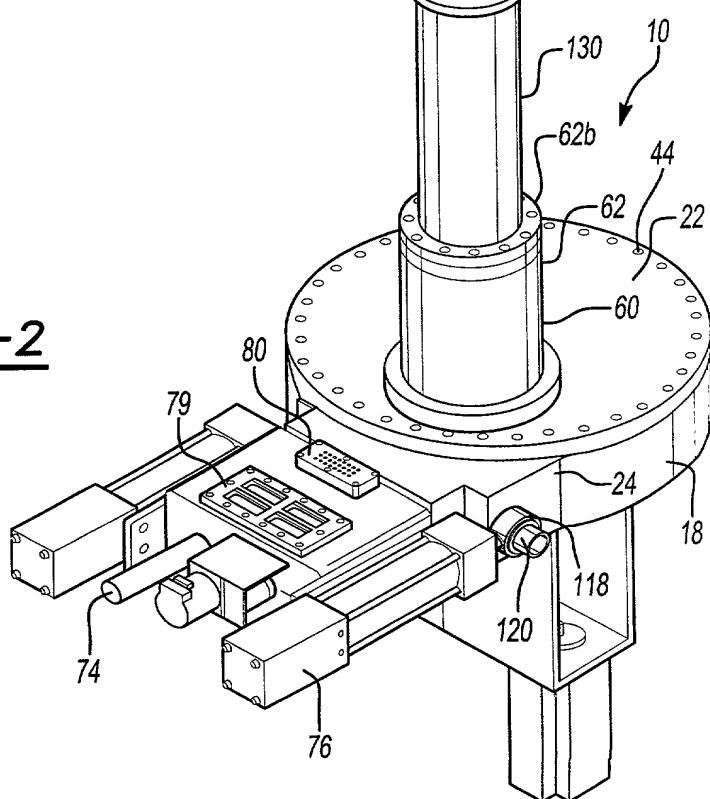


Fig-1

Fig-2



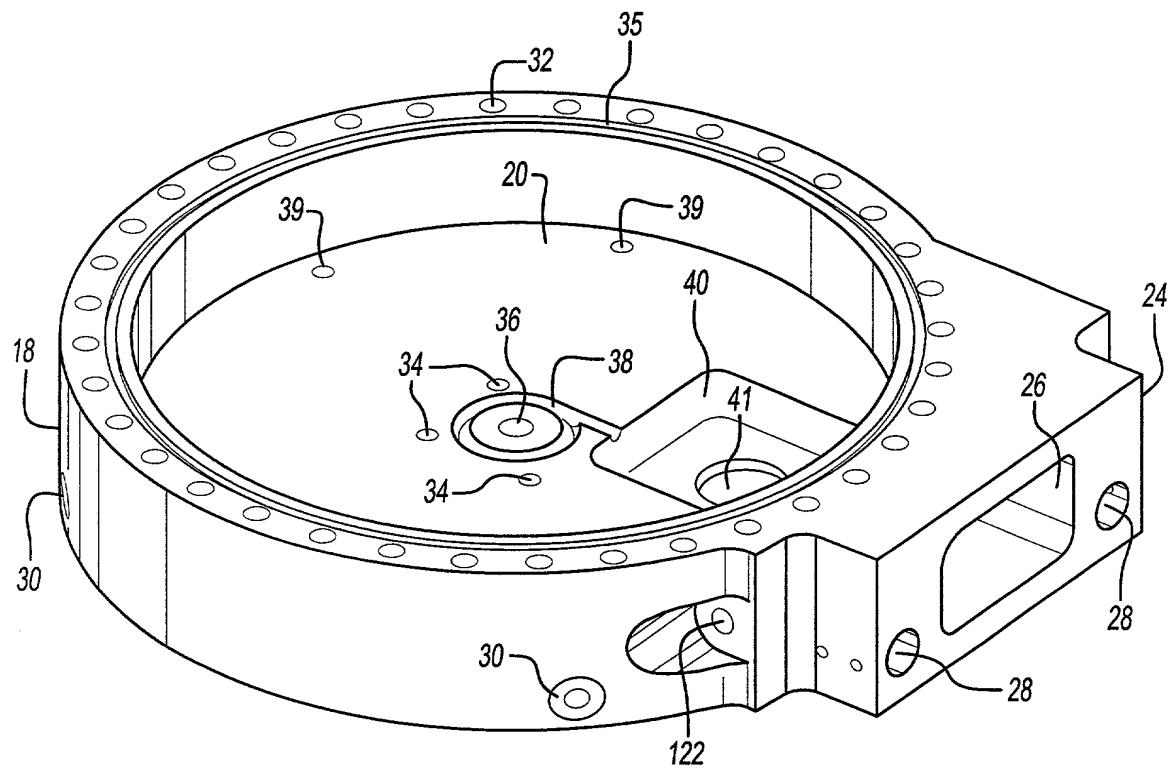


Fig-3a

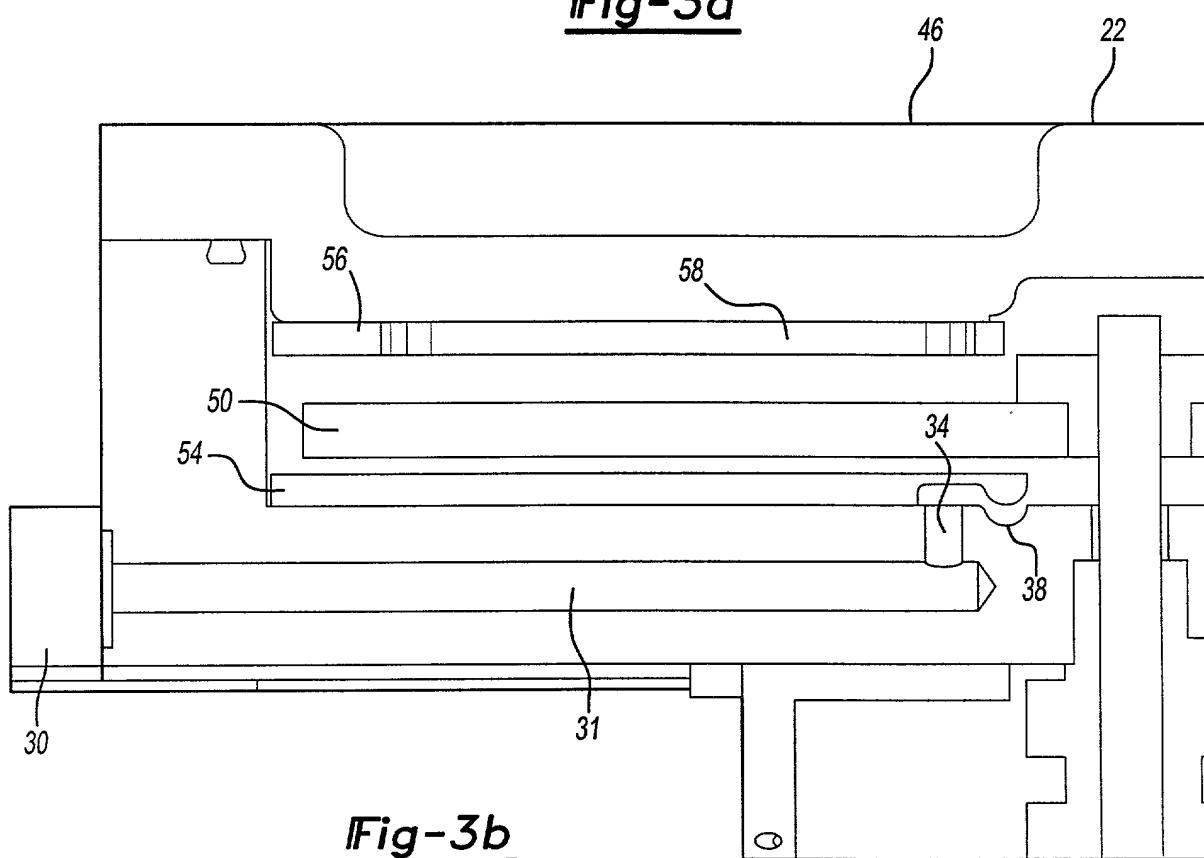
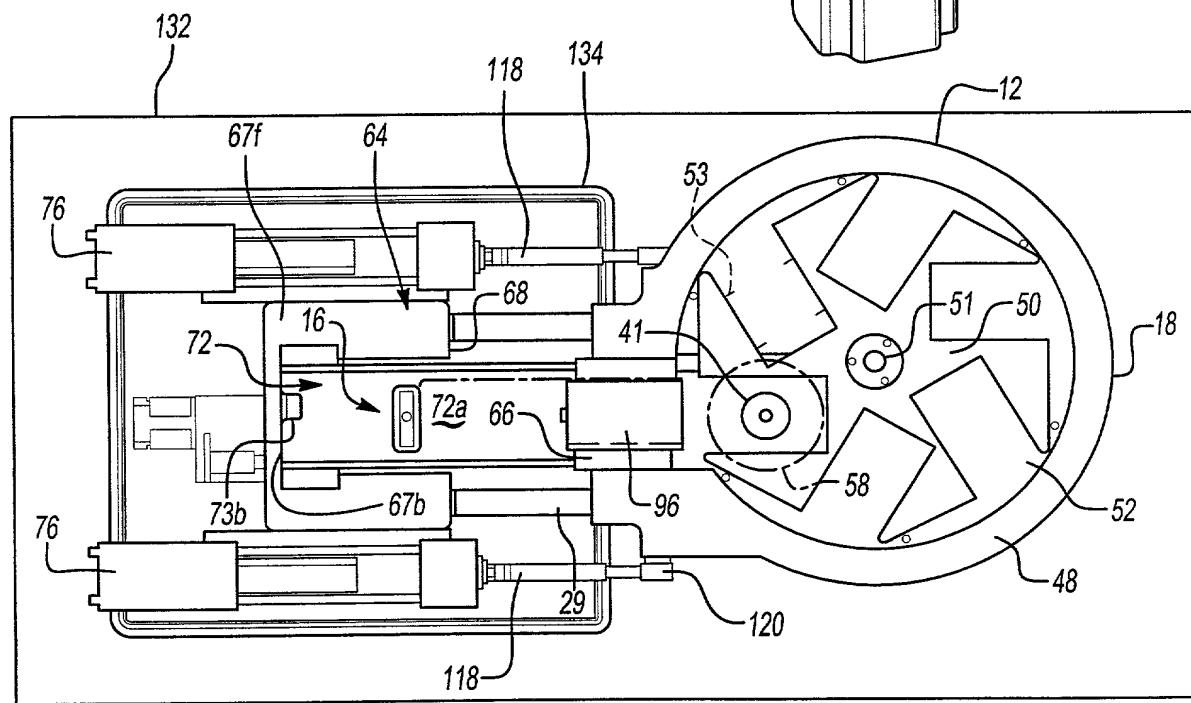
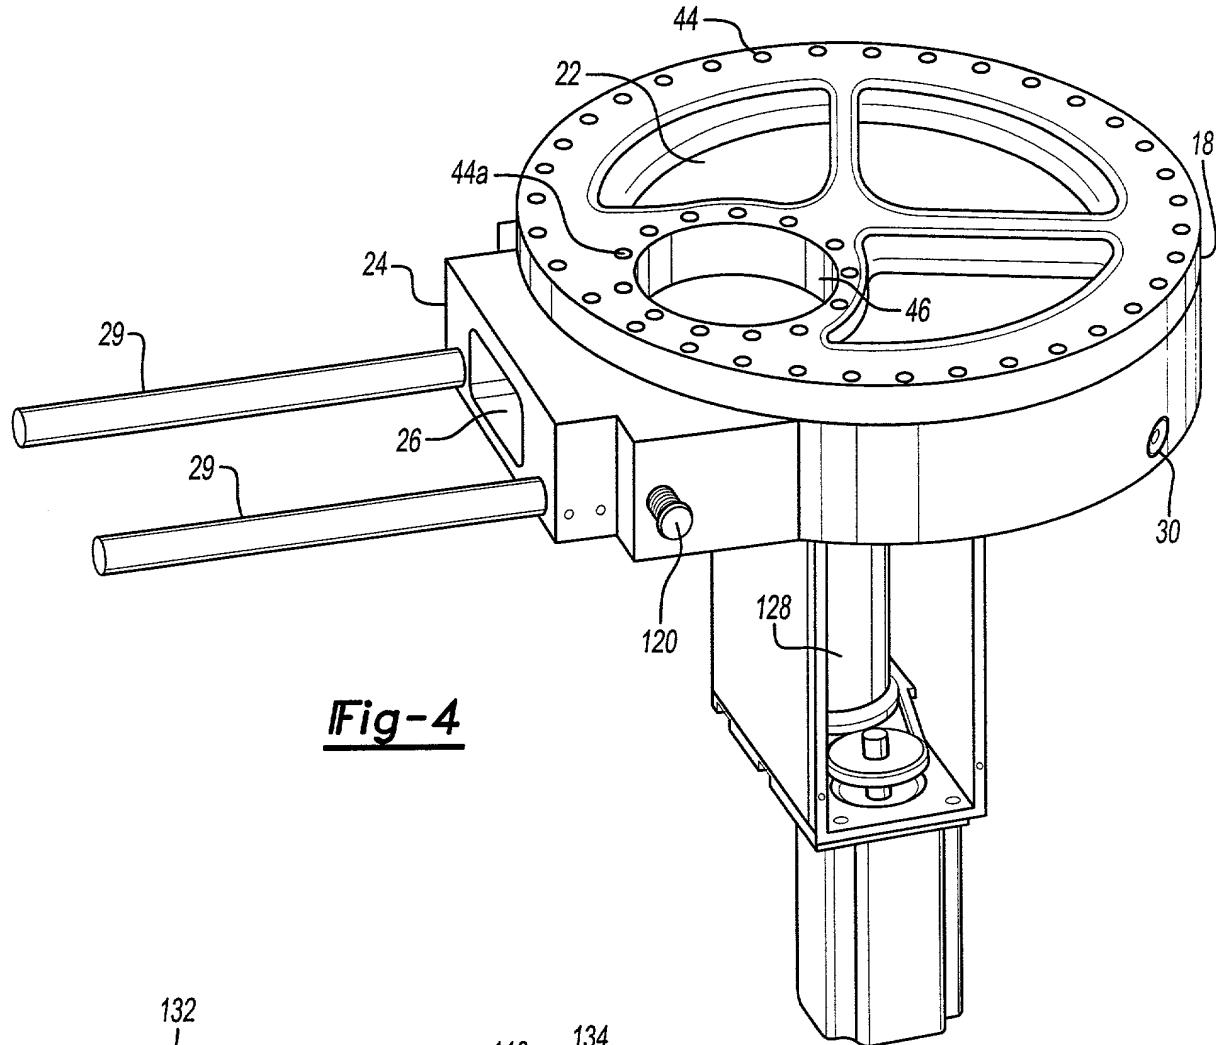


Fig-3b



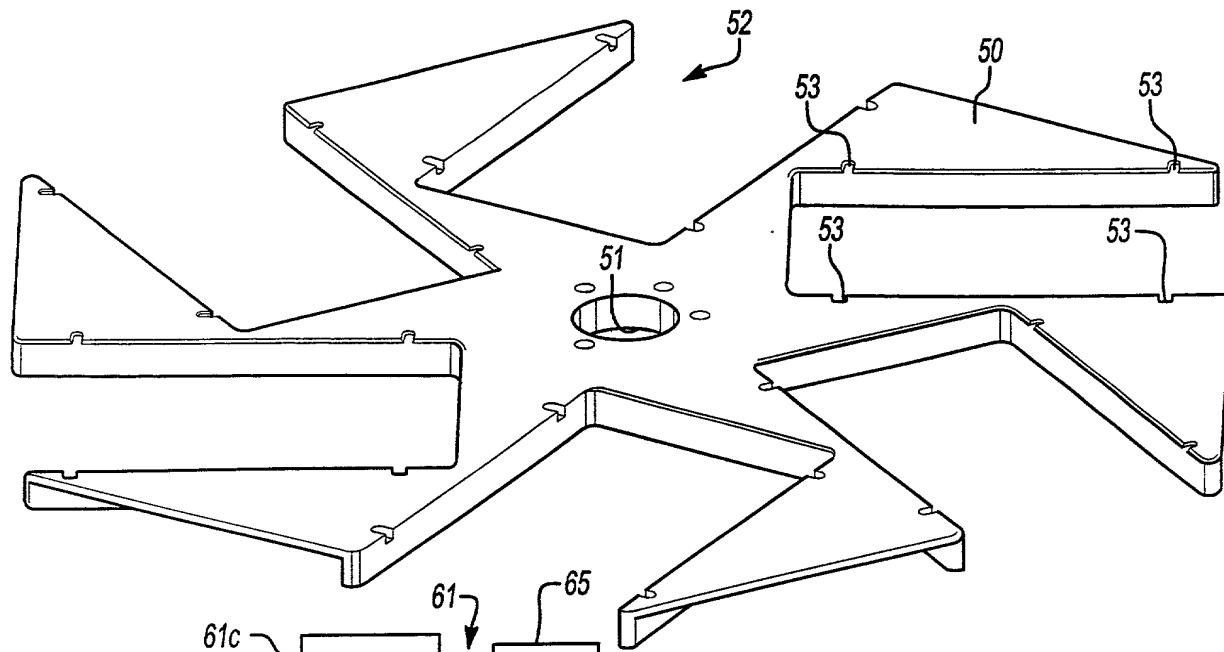


Fig-5b

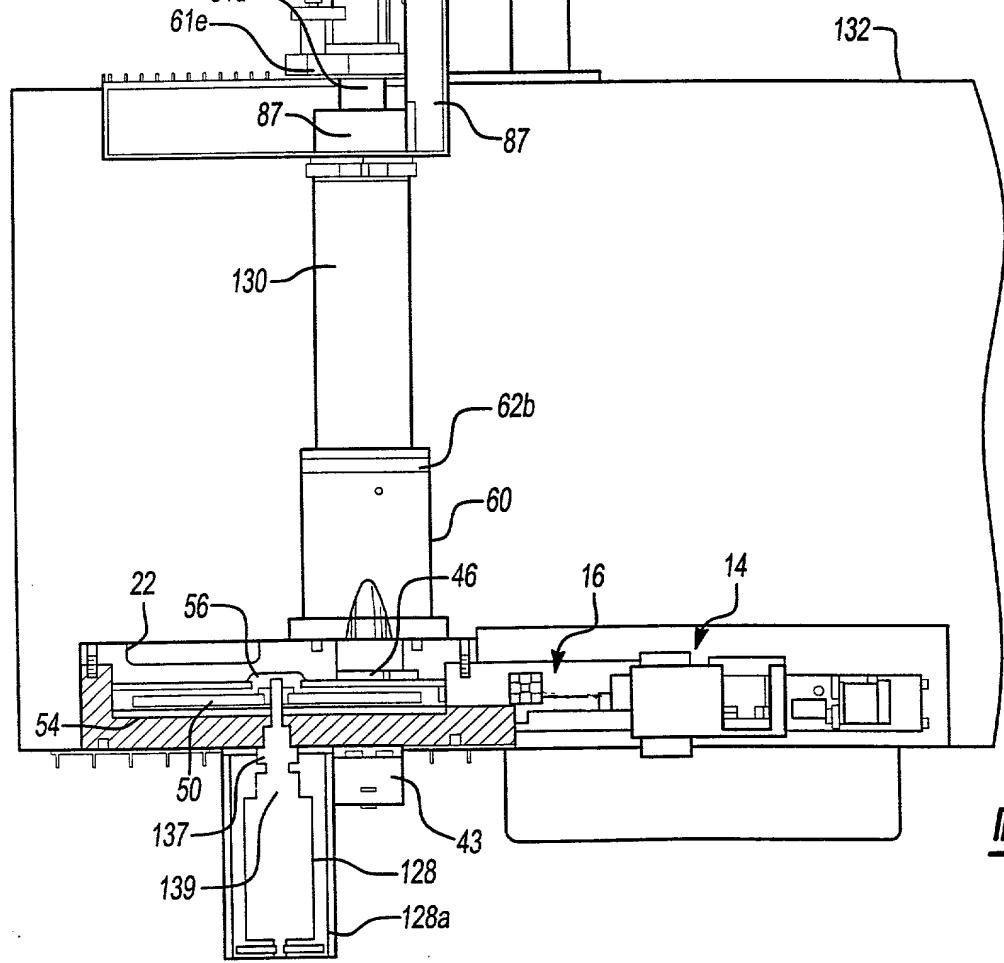


Fig-6

TITLE: IN-SITU INJECTION AND MATERIALS SCREENING DEVICE

APPLICANT: TREVOR FRANK et al.

DOCKET NO: 1012-076

5/12

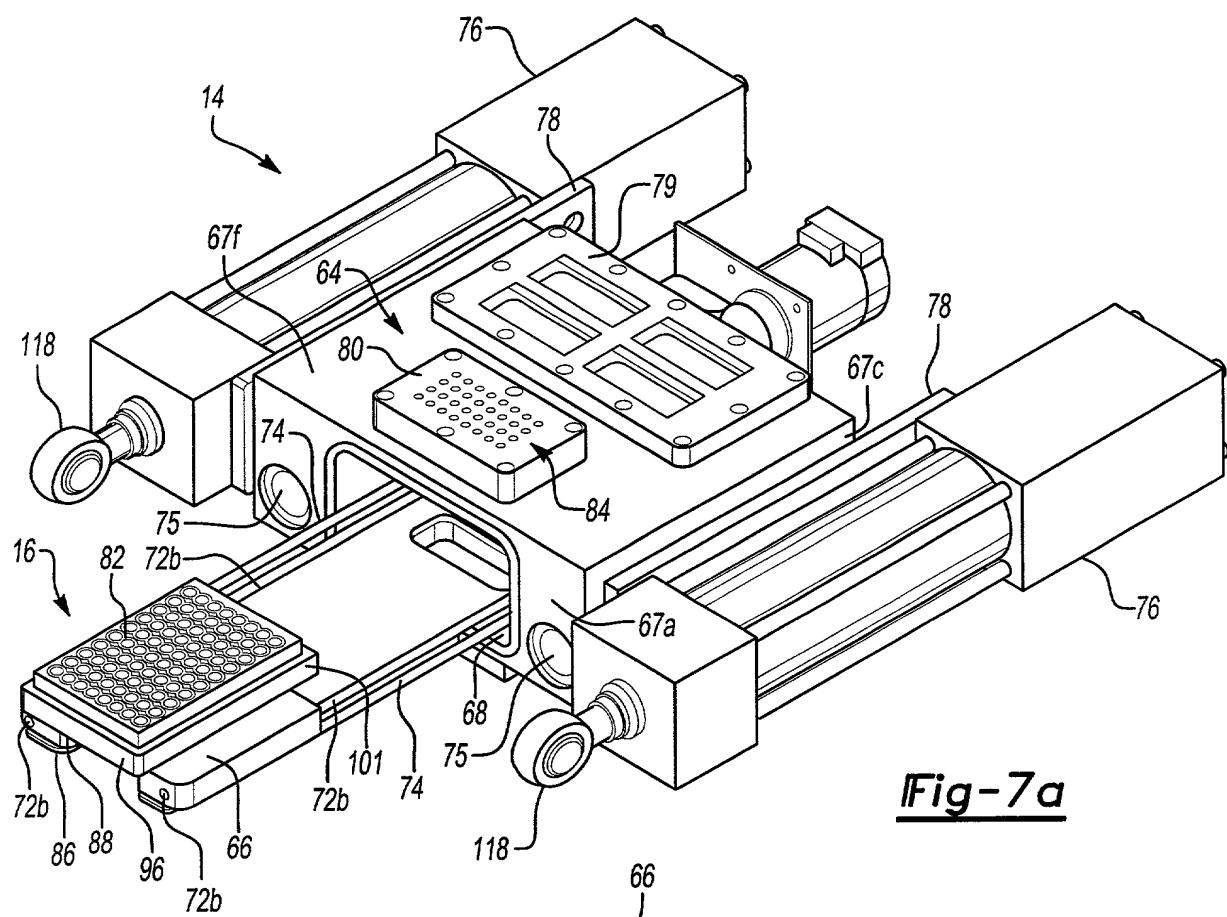


Fig-7a

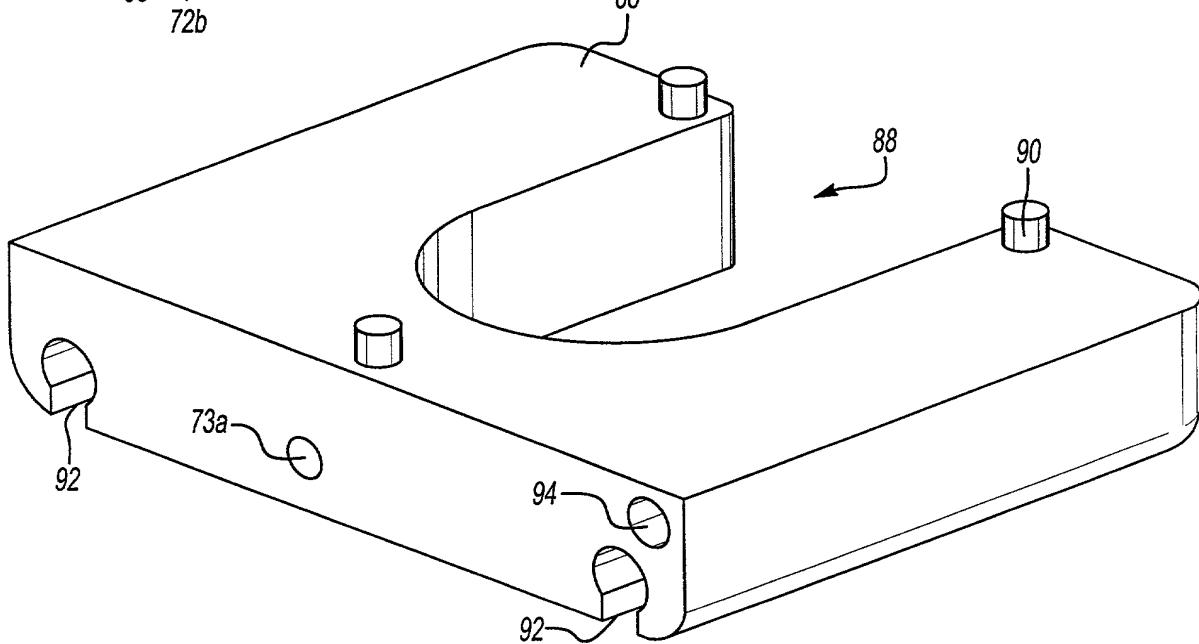


Fig-7b

TITLE: IN-SITU INJECTION AND MATERIALS SCREENING DEVICE

APPLICANT: TREVOR FRANK et al.

DOCKET NO: 1012-076

6/12

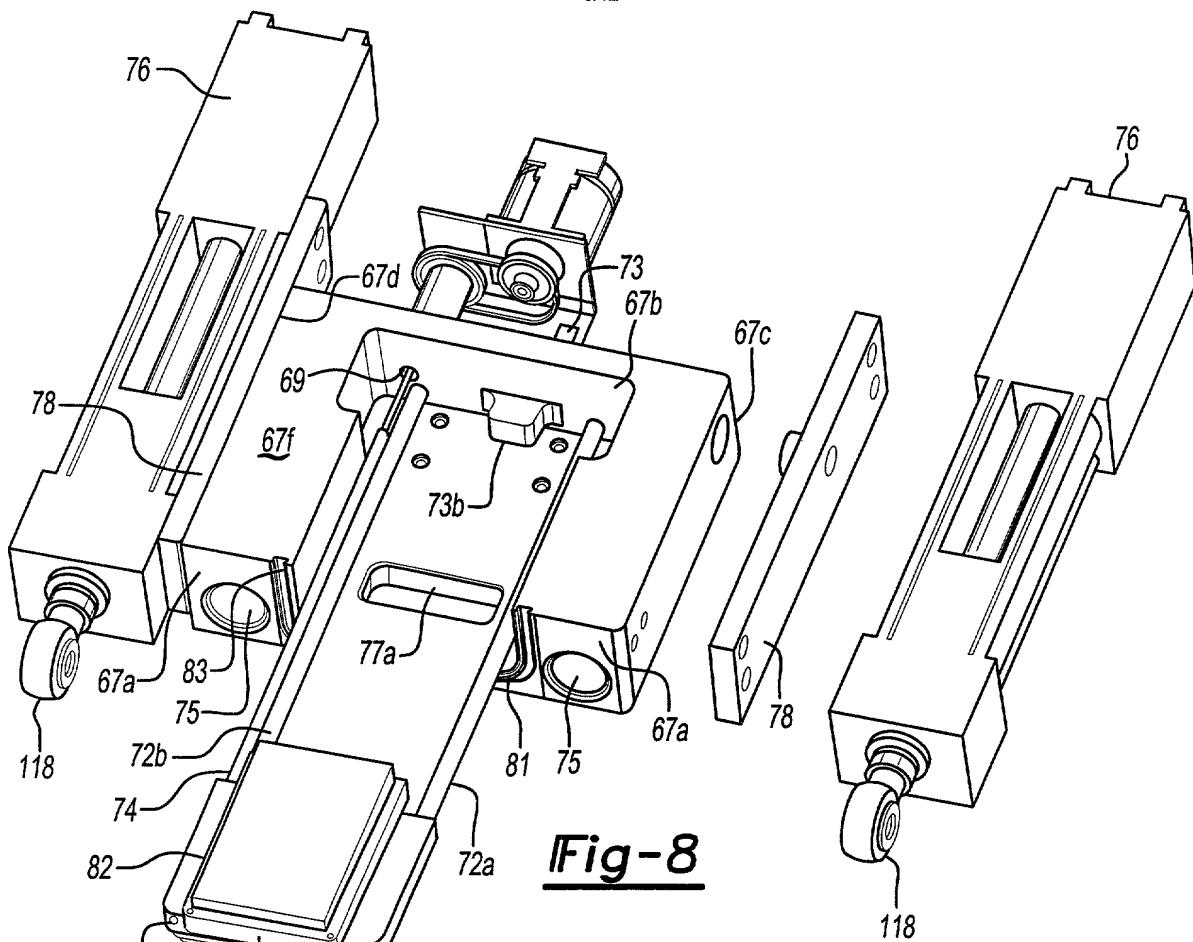


Fig-8

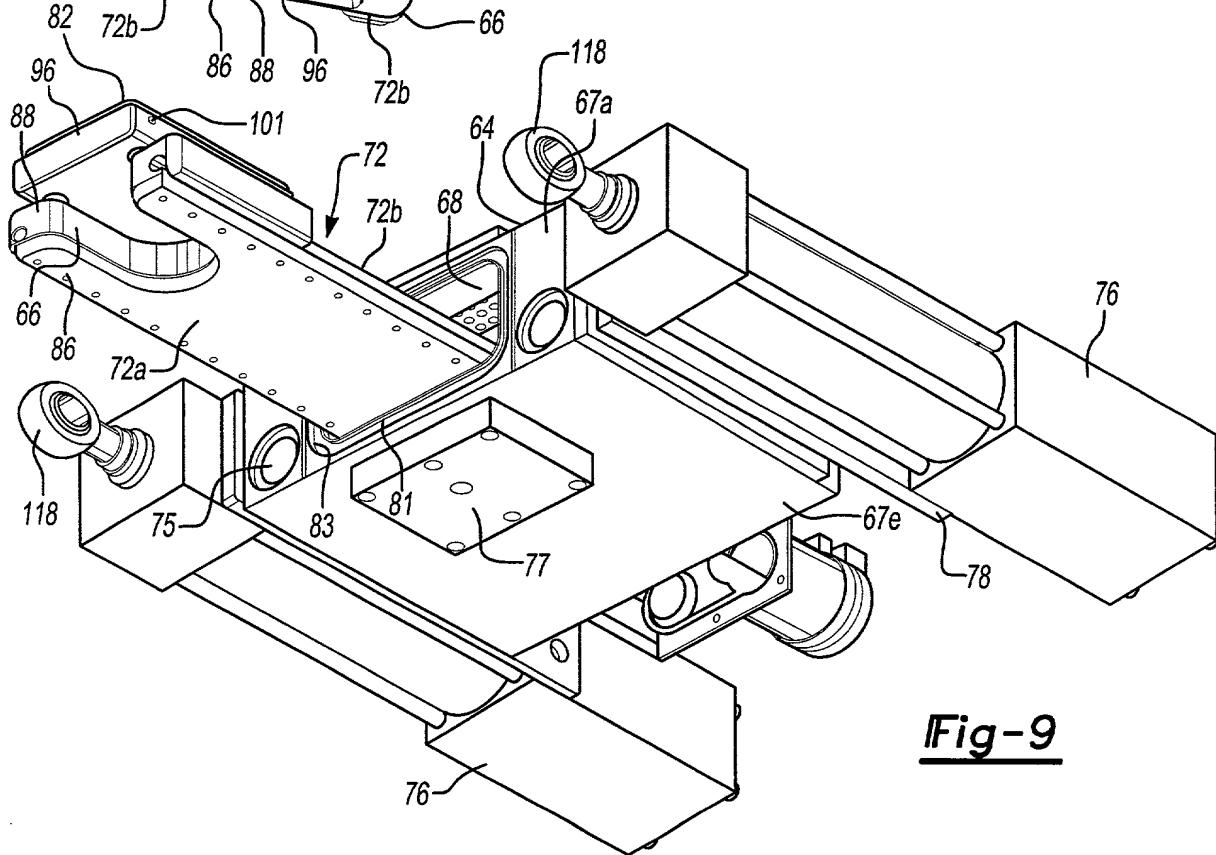


Fig-9

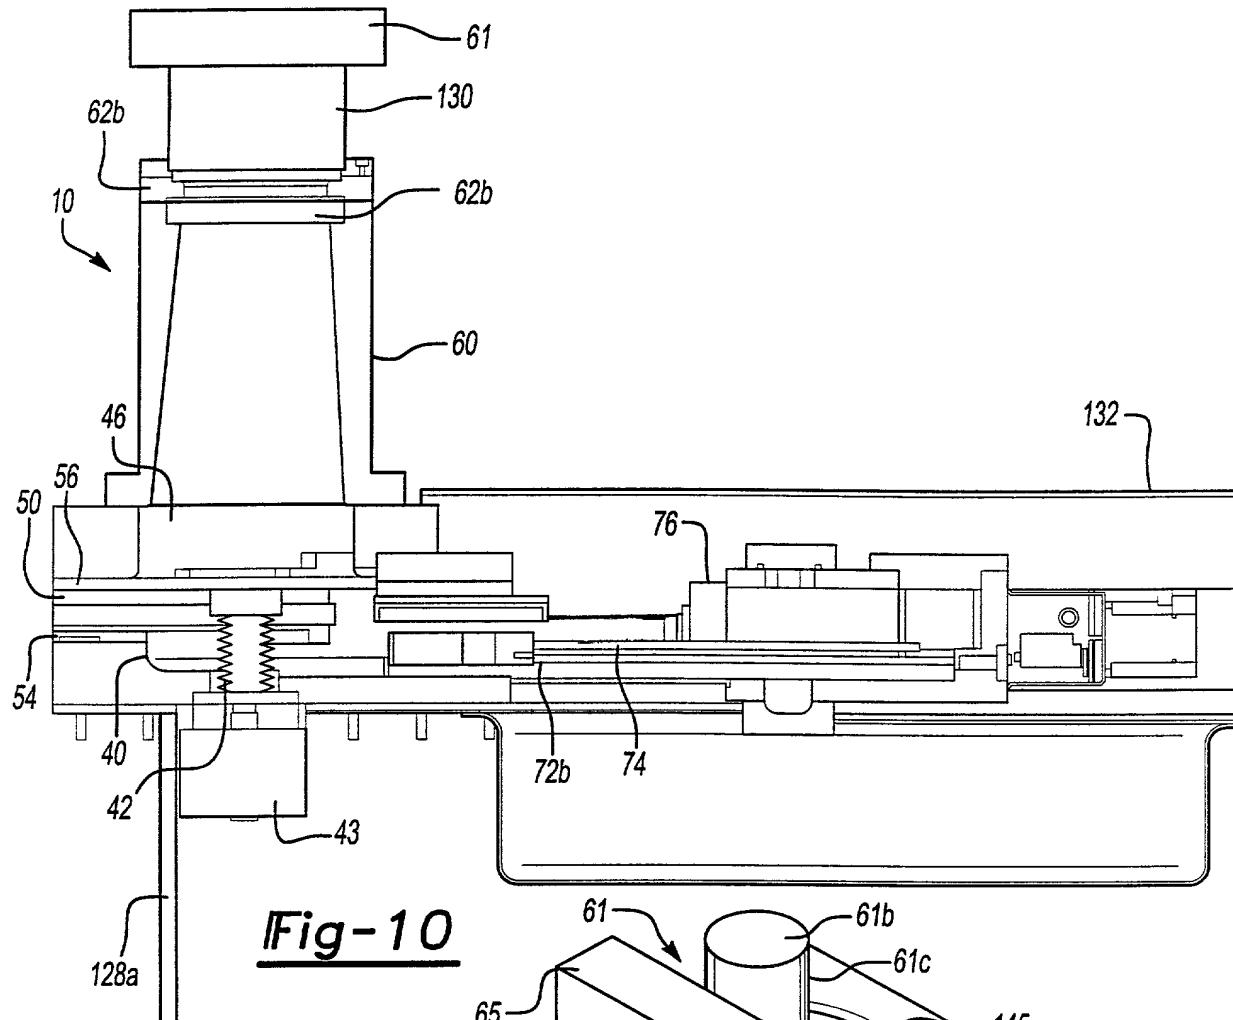


Fig-10

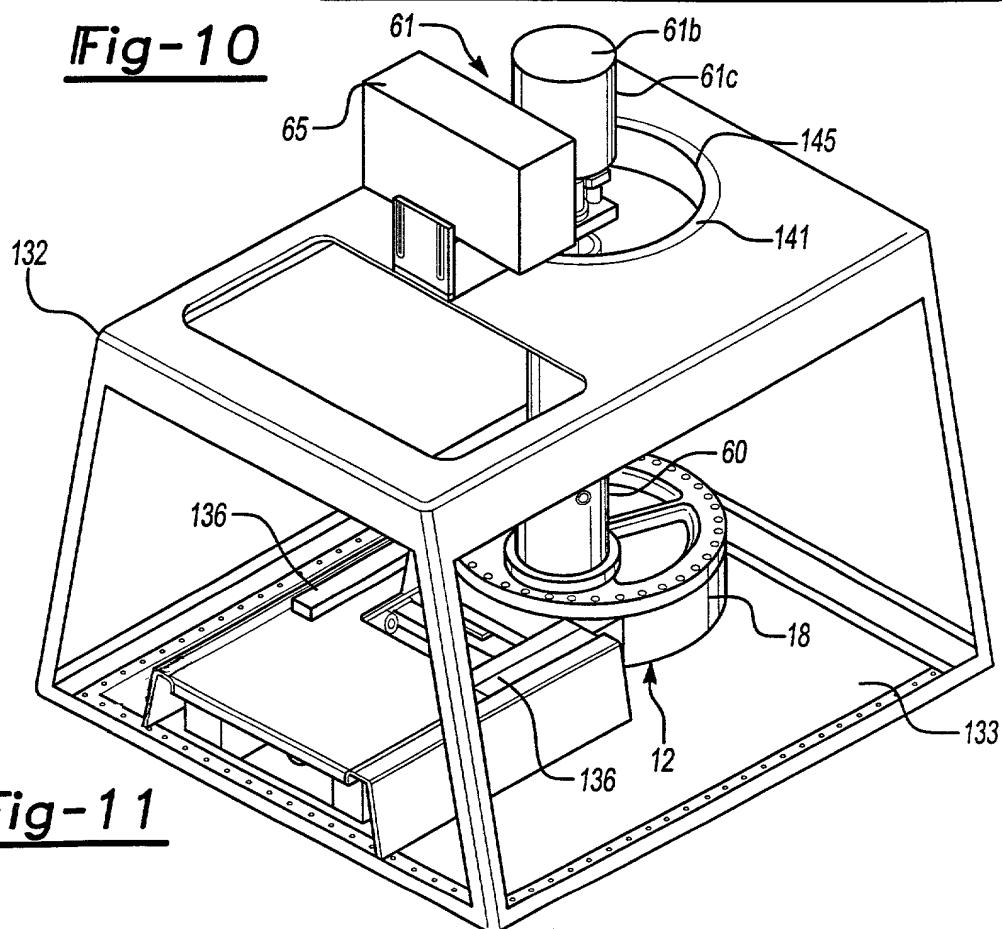


Fig-11

TITLE: IN-SITU INJECTION AND MATERIALS SCREENING DEVICE

APPLICANT: TREVOR FRANK et al.

DOCKET NO: 1012-076

8/12

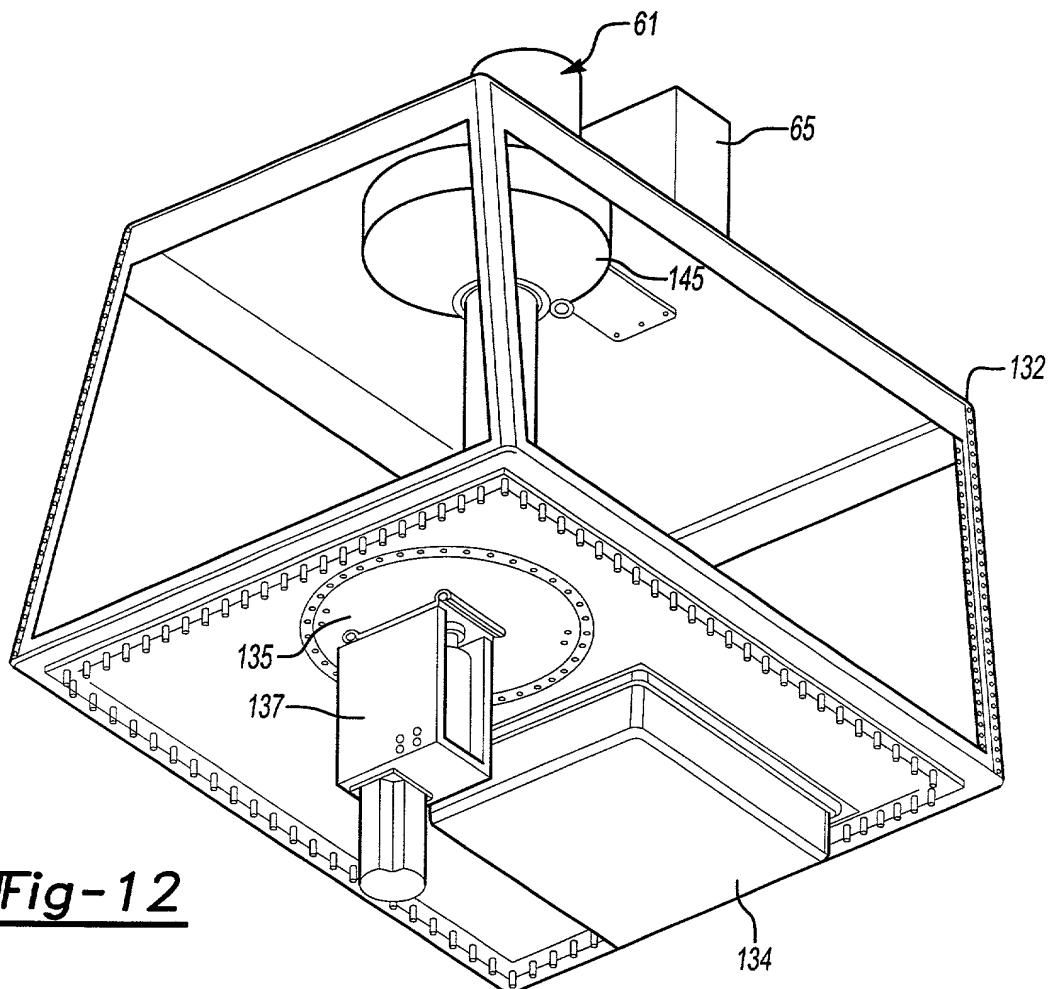


Fig-12

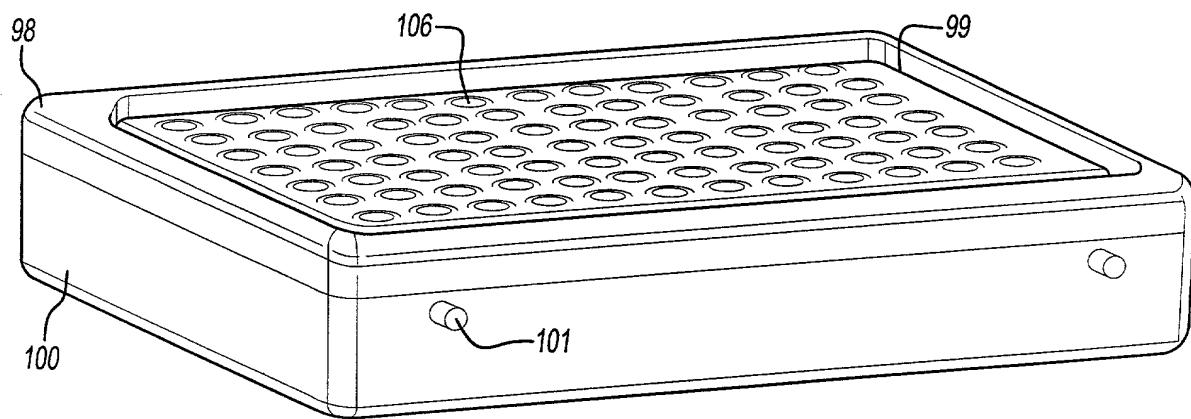


Fig-13

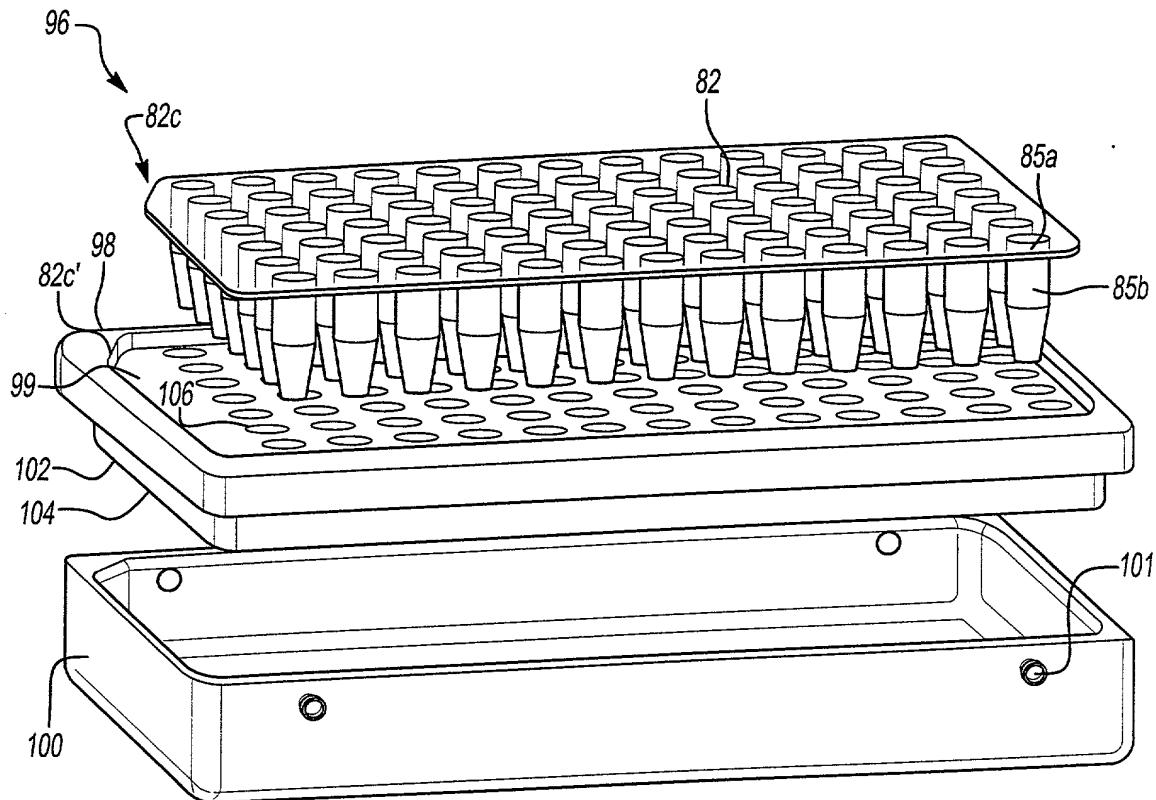


Fig-14

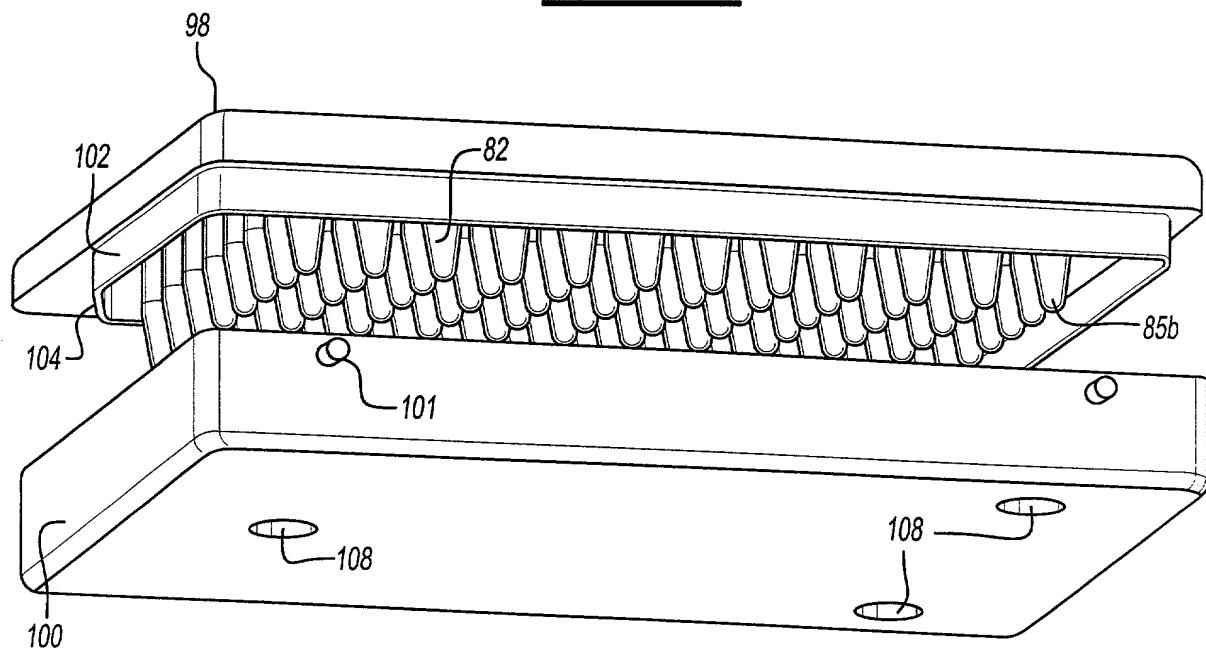


Fig-15

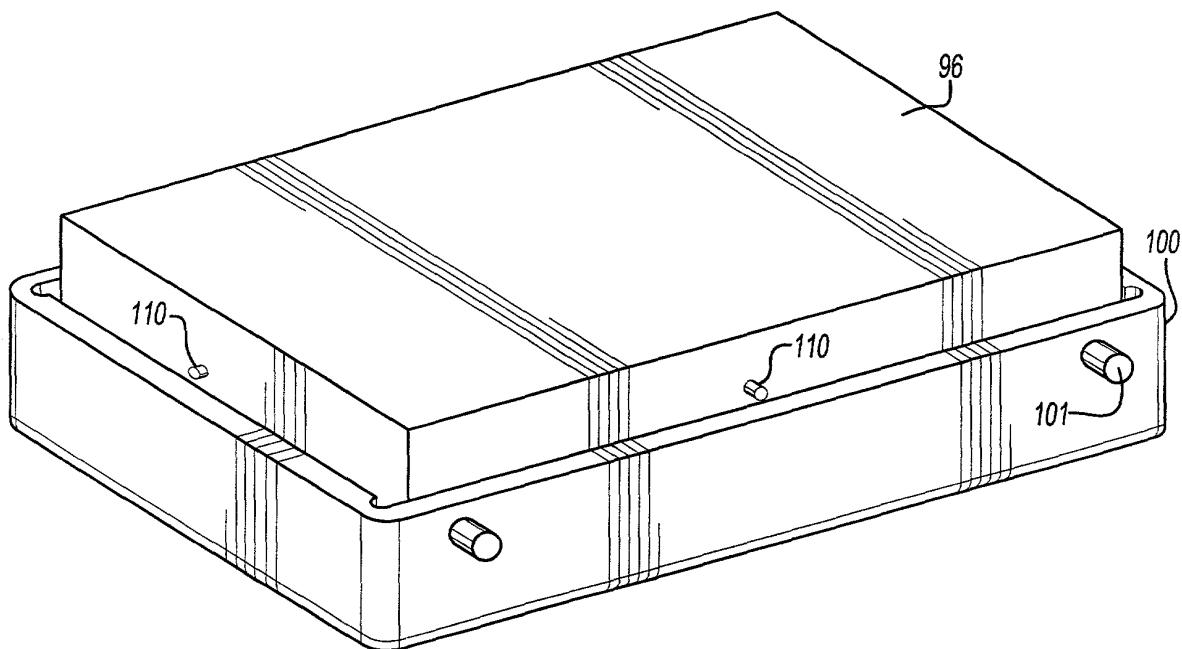


Fig-16

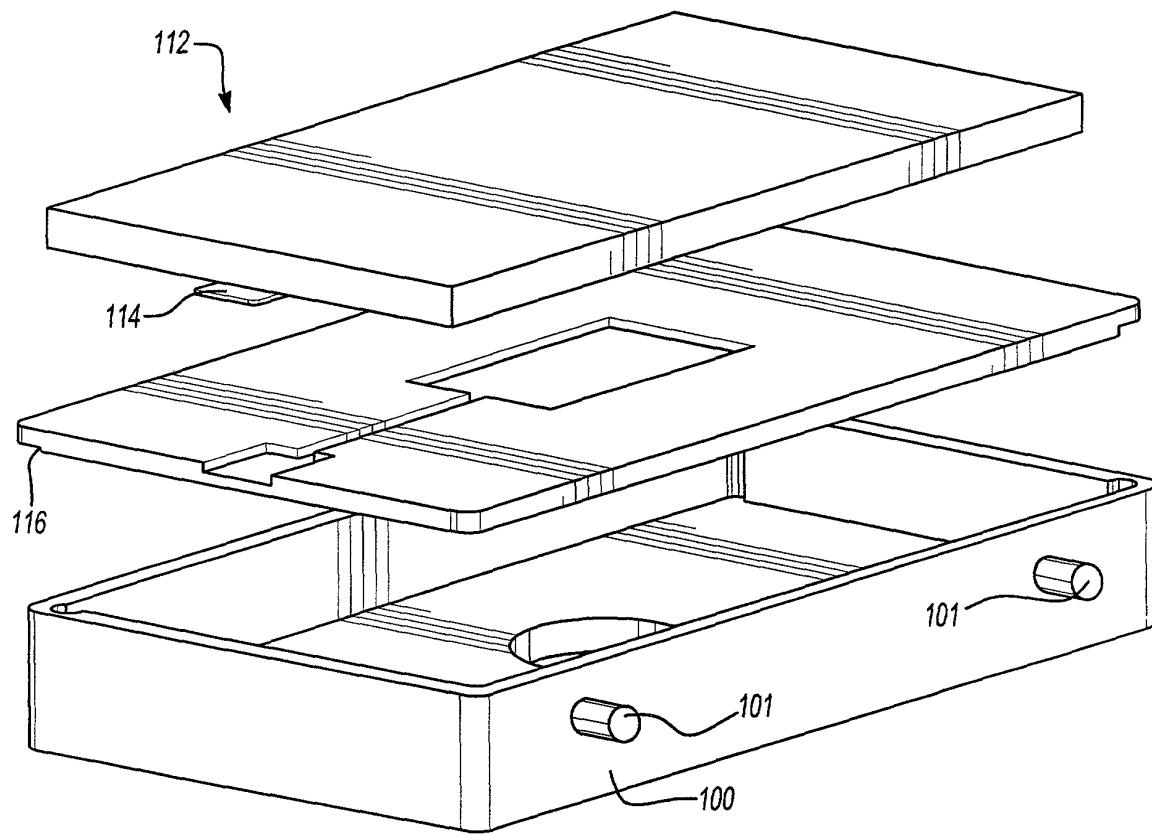
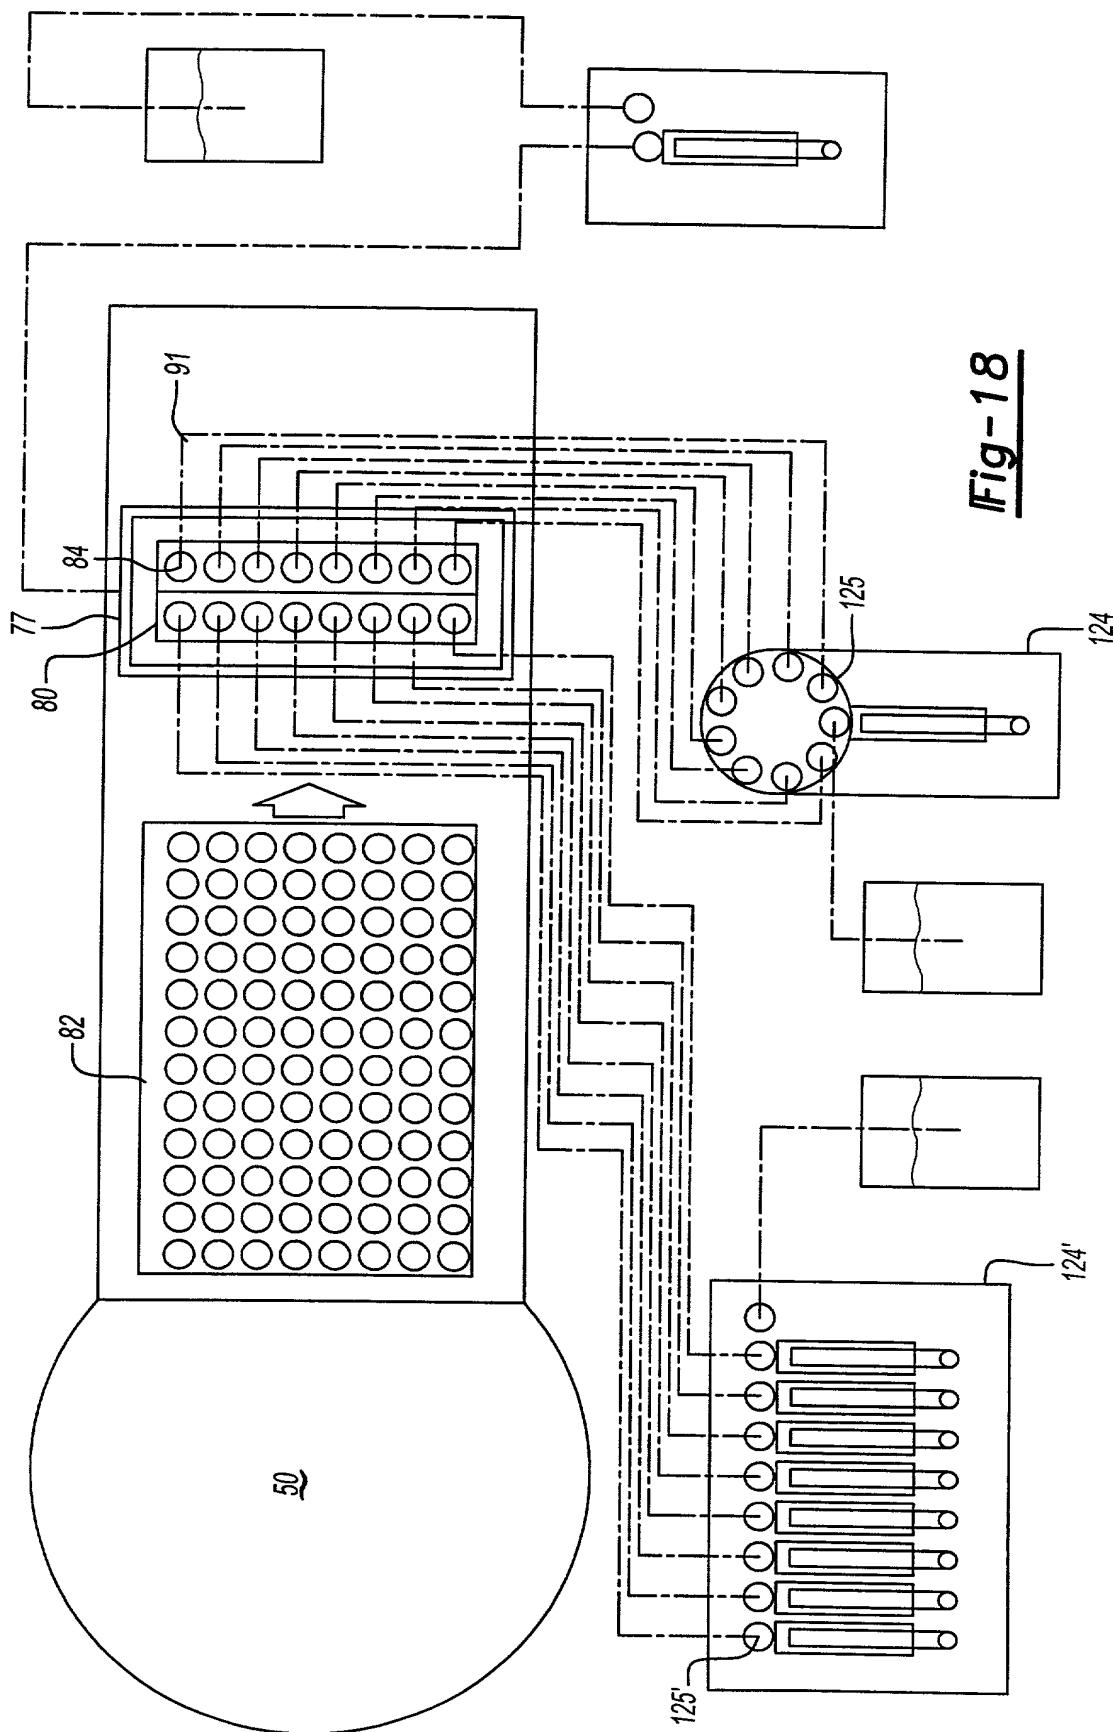


Fig-17



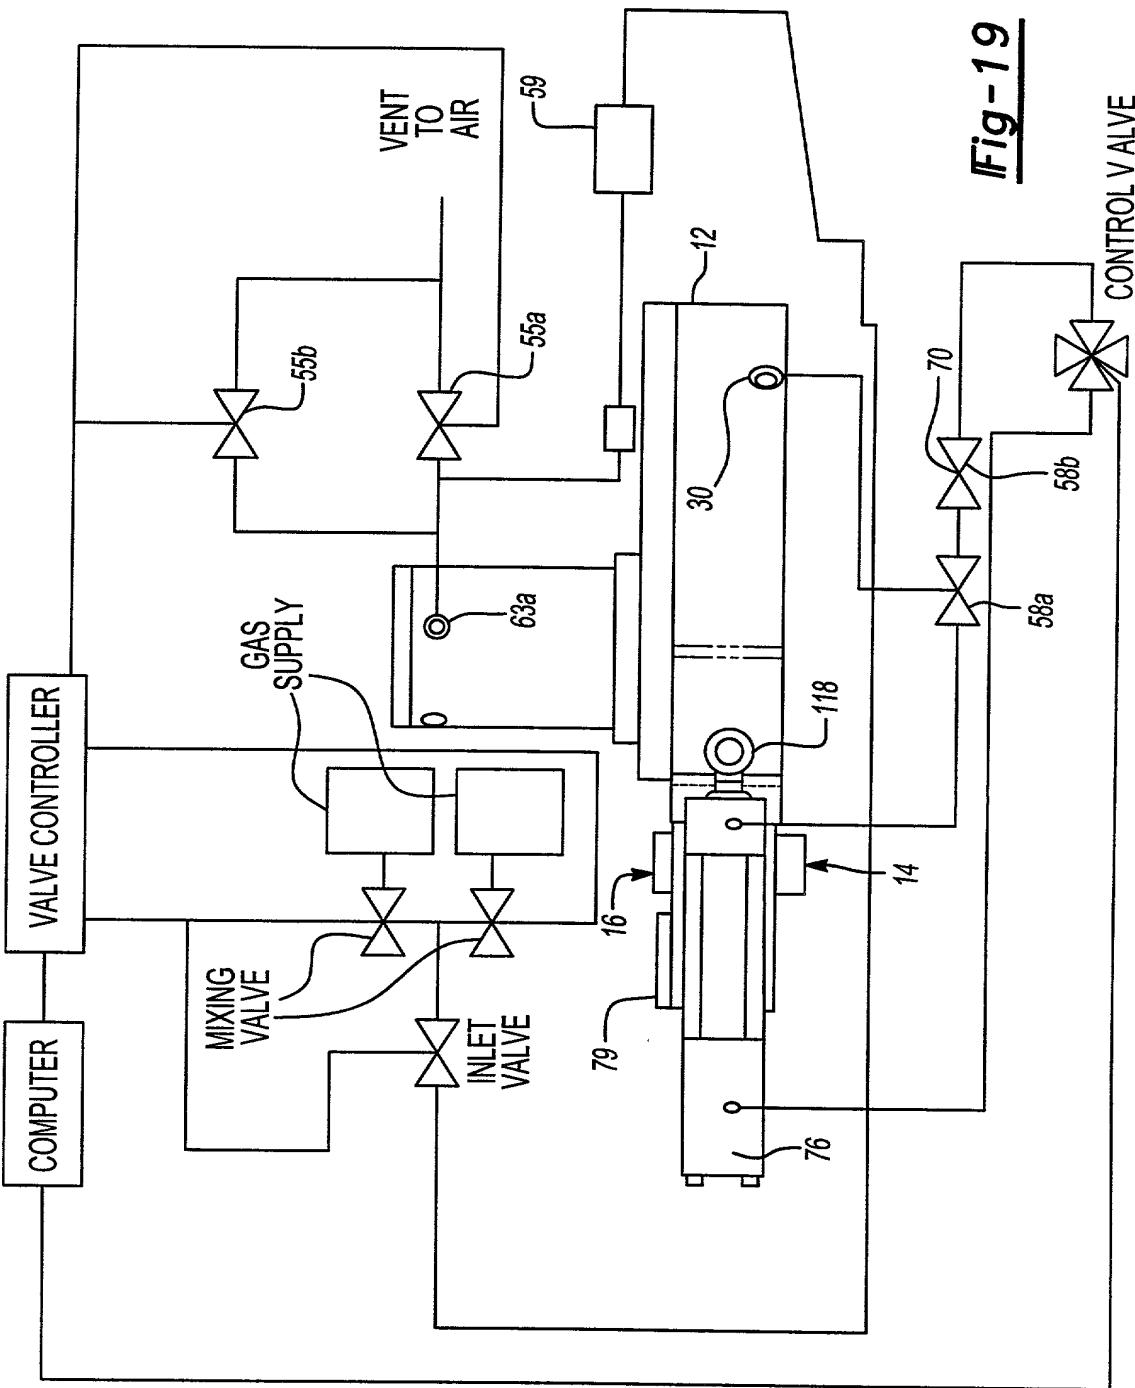


Fig - 19